


Operation Manual for Resolution Chart for Microfocus X-Ray CT Scanner

Article #: JIMA—D029—R:2022


JIMA RT CT-01B

It is greatly appreciated your purchasing JIMA RT CT-01B. Please read this operation manual well for proper usage and then, please preserve for future reference.

Appearance

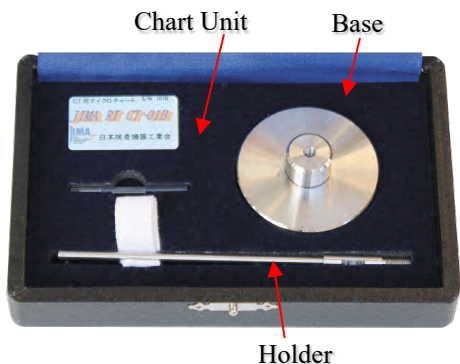


Cross section of Si Chip

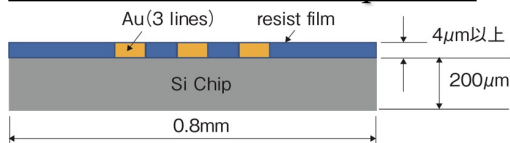

Specification


Chart Unit	Size (Polycarbonate)	φ2 × 40mm
	Si Chip	0.8x7 × 0.2mm
	Absorption Material	Gold (Au) Thickness >4 µm
	Line (T shape layout)	3 lines each, V/H
	Line/ Space Size	3,4,5,6,7 µm
	Tolerance	5 ~ 7µm: ± 10% 3 ~ 4µm: ± 15%
Holder	Size (Aluminum)	Φ 3 × 120 mm
Base	Size (Stainless Steel)	Φ 49.5 × 19 mm
Temp	Ambient OP Temp.	10°C ~ 70°C

Chart Unit

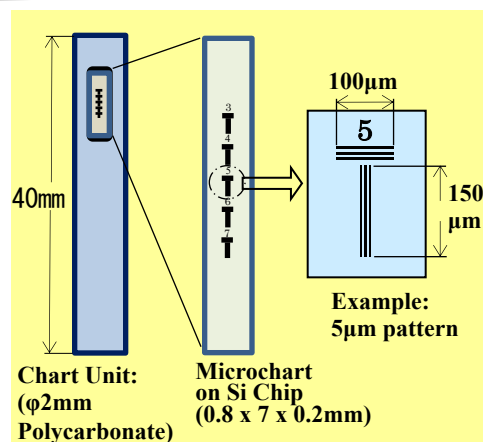

Usage

Holder and Base are included to be fixed in CT scanner if it is useful. Please try to find best way to fix.

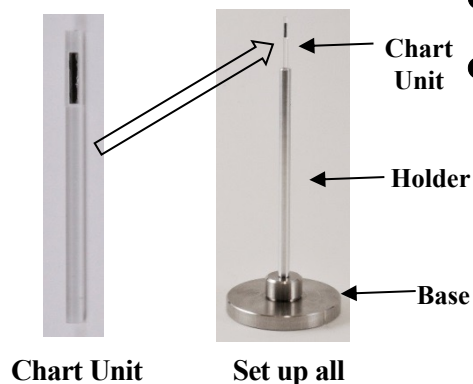

Notice of Operation

- The Resolution Chart is mounted on Si chip (0.8 x 7 mm, t=0.2 mm). Si chip is mounted in 2 mm dia. acrylic bar. The Chart thickness is only 4µm. Due to delicate construction, please avoid following handling not to damage it.
 - Do not afford pressure onto the Micro Chart.
 - Especially when Micro Chart is taken out from storage place.
 - Do not drop
 - Do not immerse in liquid nor chemical.
- When Chart Unit is fixed onto Holder, please adjust with tape if it is loose.
- Do not disassemble the aluminum holder at all.
 - The ability of the test sample cannot be maintained if disassembled.
 - Once disassembled, it is impossible to assemble again.
- This product will be supplied in an air-cushioned case. However, due to delicate precise construction, please handle with care not to put strong impact such as dropping even in the case.
- Please use under +10 degree C to +70 degree C ambience temperature.
- Please storage under controlled circumstances. Recommended range is Temperature 23 +/- 5 degree C, humidity: 50 +/- 10%
- Please use this products to maintain capability of X-Ray systems.
- This product cannot be measure line width after assembled nor cannot be re-certified.
- This product is a kind of expendable supply. It cannot be repaired nor re-assembled
- After receipt of goods, please check any outside damage and test with X-Ray without delay. We cannot accept any claim after one month from delivery. If any defect, we will replace it.
- X-Ray imaging software is different depend on manufacturer. The image might be reversed.
- The thickness of absorption material may be different at point to point. This may cause variation of shading in the image.

General Corporation Japan Inspection Instruments Manufacturers' Association



3rd. Fl., Kudan Royal Bldg., 3-2-5 Kandajinbo-cho,
Chiyoda-ku, Tokyo 101-0051 Japan

TEL 03-3288-5080 FAX 03-3288-5081

E-mail rtp@jima.jp URL <http://www.jima.jp>